

Gyrolab® Assays

Human IL-10 Assay


INTRODUCTION

Interleukin 10 (IL-10) is a potent anti-inflammatory cytokine that plays an essential role in limiting the excessive inflammatory and autoimmune responses triggered by pathogens, thereby preventing damage to the normal tissue.

We have developed a three-step sandwich Gyrolab assay to determine IL-10 in human serum samples. Use of this protocol on Gyrolab systems will reduce time to market and increase productivity while maintaining quality requirements.

ASSAY DESIGN

The assay was set up as a three-step sandwich assay with biotinylated anti-human IL-10 monoclonal antibody as a capture molecule and an anti-human IL-10 monoclonal antibody labeled with Alexa Fluor® 647 as a detection molecule. Recombinant human IL-10 (rh IL-10) was used as standard material.

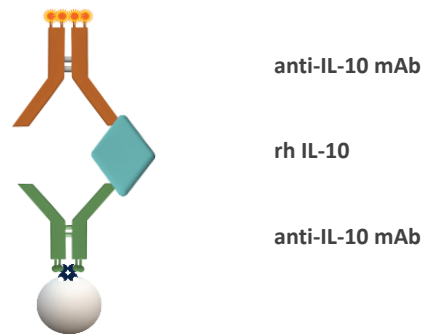

ASSAY PERFORMANCE

Dynamic range, accuracy and precision

A robust 4-log standard curve (Figure 1) was generated over three runs, achieving an assay range from 1 pg/mL to 1 500 pg/mL (Table 1). The Limit of Detection (LOD) was determined as the concentration corresponding to at least two standards deviations above the assay blank.

The inter-run precision (CV, Coefficient of Variation), established with QC samples over the assay range run in triplicate in three runs, was <20% (Table 2).

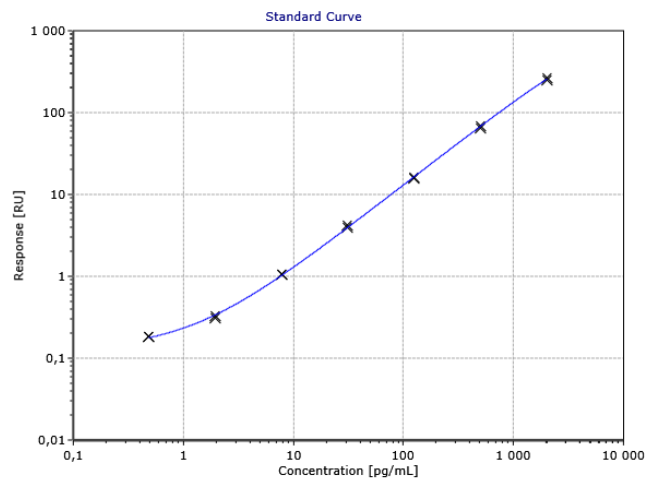


Figure 1 Standard curve in REXIP® H

Table 1 Estimated Assay Range, based on three runs

Assay range	LOD (pg/mL)	LLOQ (pg/mL)	ULOQ (pg/mL)
On plate	~ 0.6	~ 1	~ 1 500
In neat matrix	~ 1.2	~ 2	~ 3 000

Table 2 Accuracy and precision data of QC samples in REXXIP H, n = number of runs

QC	Expected Conc (pg/mL)	Average Measured Conc (pg/mL)	Inter Run CV (%; n=3)	Average Intra Run CV (%; n=3)	Average Total Error (%; n=3)
1	1	1.0	13	13	22
2	2	2.2	3.5	7.4	15
3	10	11	8.6	3.4	13
4	25	27	3.2	2.5	10
5	100	103	0.72	3.0	5.5
6	1 500	1 572	2.7	3.5	8.4

Dilution linearity

Linearity of dilution was examined by spiking human recombinant IL-10 into human serum samples. The spiked serum samples were diluted 1:2 in REXXIP H-max and then serially diluted 1:2 in REXXIP H (1:4-1:64) to obtain six data points (Table 3).

Table 3 Linearity of dilution. Each dilution was analyzed in triplicate

Sample	Dilution Factor	Calculated Conc (pg/mL)	CV	Recovery (%)
			(%)	
1	2	580	1.2	109
	4	559	1.4	105
	8	557	5.3	105
	16	554	3.6	104
	32	553	2.5	104
	64	529	4.6	99
2	2	512	4.2	96
	4	529	1.9	99
	8	532	4.3	100
	16	527	2.0	99
	32	507	1.8	95
	64	501	6.3	94
3	2	526	1.0	99
	4	495	4.1	93
	8	481	0.72	90
	16	480	0.73	90
	32	480	2.9	90
	64	477	1.2	90

Parallelism

Parallelism tests could not be performed since the endogenous level of human IL-10 was below the quantification range. It is recommended that end users assess parallelism when suitable samples with significant levels of analyte are identified.

MATERIALS AND METHODS

The assay was developed on a Gyrolab xP system using Gyrolab® Bioaffy™ 4000 CD. The assay was set up using a three-step method with two wash solutions (4000-3W-001-A) and a 5% PMT setting. The assay buffer was Rexpip H. The Minimum Required Dilution (MRD) for serum samples was 1:2. Biotinylated rat monoclonal anti-human IL-10 antibody (clone 12G8) from Mabtech was used in a concentration of 100 µg/ml diluted with PBS-T.

The detection antibody, labeled with Alexa Fluor® 647 according to the Gyrolab standard protocol (Gyrolab User Guide), was a rat monoclonal anti-human IL-10 antibody (clone 9D7) from Mabtech, diluted to 25 nM in Rexpip F. The assay standard used was recombinant human IL-10 from R&D Systems (catalogue no. 217-IL). The standard curve was prepared in Rexpip H.

Summary table

Capture	Biotinylated rat monoclonal anti-human IL-10 antibody (clone 12G8, Mabtech, 3430-6-250), diluted to 100 µg/mL in PBS-T + 0.02% sodium azide
Detection	Rat monoclonal anti-human IL-10 antibody (clone 9D7, Mabtech, 3430-2-250) labeled with Alexa Fluor® 647, 25 nM in Rexpip® F
Analyte	Recombinant human IL-10 (R&D Systems, 217-IL) in Rexpip® H
CD-type	Gyrolab® Bioaffy™ 4000
Method	4000-3W-001-A
Wash buffer for needles	Wash buffer 1: PBS-T Wash buffer 2: Gyrolab Wash Buffer pH 11
PMT-setting	5%
Expected dynamic range	Approximately 1 pg/mL to 1 500 pg/mL (2 pg/mL to 3 000 pg/mL in neat human serum, dilution 1:2)

Recommendations

When developing this assay, it is important to screen matrices and assess backgrounds, in particular for the specific disease matrices. Parameters, such as LLOQ, should be validated in-house. Data given in this document should only be considered as guidance.

For additional support contact your local Field Application Support

Gyrolab and Rexpip are registered trademarks and Gyros, Gyrolab xPlore, Gyroplex, Bioaffy and Gyros logo are trademarks of Gyros Protein Technologies Group. All other trademarks are the property of their respective owners. Products and technologies from Gyros Protein Technologies are covered by one or more patents and/or proprietary intellectual property rights. All infringements are prohibited and will be prosecuted. Please contact Gyros Protein Technologies AB for further details. Products are for research use only. Not for use in diagnostic procedures. © Gyros Protein Technologies AB 2021. D0037461/B