

Gyrolab® Assays

Human IL-1beta Assay


INTRODUCTION

Interleukin 1beta (IL-1 β) is a major pro-inflammatory cytokine that is essential for host-defence responses to infection and tissue injury. It exerts pleiotropic effects on both the innate and adaptive immune system. IL-1 β play key roles in acute and chronic inflammatory response, it also exacerbates damage during autoimmune, autoinflammatory and degenerative diseases, including cancer.

We have developed a three-step sandwich Gyrolab assay to determine IL-1 β in human serum samples. Use of this protocol on Gyrolab systems will reduce time to market and increase productivity while maintaining quality requirements.

ASSAY DESIGN

The assay was set up as a three-step sandwich assay with biotinylated anti-human IL-1 β monoclonal antibody as a capture molecule and an anti-human IL-1 β polyclonal antibody labeled with Alexa Fluor® 647 as a detection molecule. Recombinant human IL-1 β (rh IL-1 β) was used as standard material.

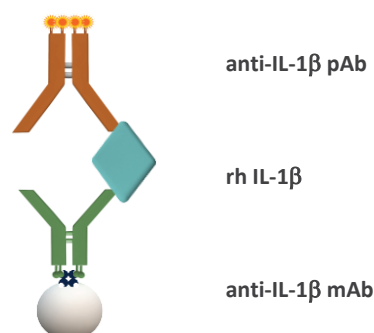

ASSAY PERFORMANCE

Dynamic range, accuracy and precision

A robust 3 to 4-log standard curve (Figure 1) was generated over three runs, achieving an assay range from 1 pg/mL to 1 000 pg/mL (Table 1). The Limit of Detection (LOD) was determined as the concentration corresponding to at least two standards deviations above the assay blank.

The inter-run precision (CV, Coefficient of Variation), established with QC samples over the assay range run in triplicate in three runs, was <20% (Table 2).

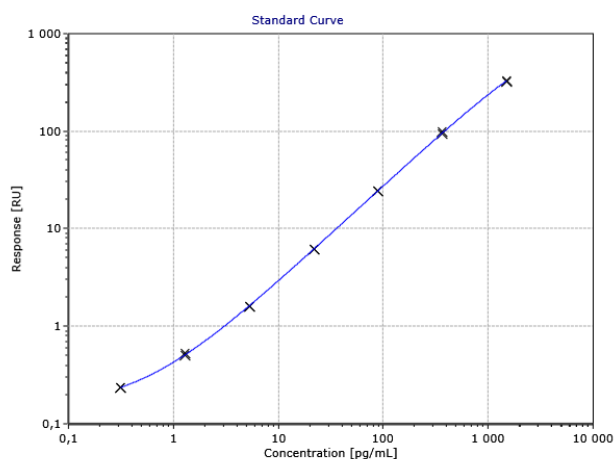


Table 1 Estimated Assay Range, based on three runs

Assay range	LOD (pg/mL)	LLOQ (pg/mL)	ULOQ (pg/mL)
On plate	~ 0.5	~ 1	~ 1 000
In neat matrix	~ 1	~ 2	~ 2 000

Figure 1 Standard curve in REXIP® H

Table 2 Accuracy and precision data of QC samples in REXXIP H, n = number of runs

QC	Expected Conc (pg/mL)	Average Measured Conc (pg/mL)	Inter Run CV (%; n=3)	Average Intra Run CV (%; n=3)	Average Total Error (%; n=3)
QC 1	1	1.1	14	7.4	20
QC 2	3	3.1	6.4	5.4	9.5
QC 3	50	51	6.6	3.5	8.9
QC 3	750	789	7.6	3.6	9.7
QC 4	1 000	1 013	5.9	2.1	6.5

Dilution linearity

Linearity of dilution was examined by spiking recombinant human IL-1 β into human serum samples. The spiked serum samples were diluted 1:2 in REXXIP H-max and then serially diluted 1:2 in REXXIP H (1:4-1:64) to obtain six data points (Table 3).

Table 3 Linearity of dilution. Each dilution was analyzed in triplicate.

Sample	Dilution Factor	Calculated Conc (pg/mL)	Recovery (%)	CV (%)
Human serum pool	2	188	102	1.3
	4	190	103	5.8
	8	180	98	3.3
	16	184	100	6.4
	32	175	95	2.3
	64	177	96	5.9
Human serum individual 1	2	170	93	4.2
	4	177	96	1.3
	8	182	99	1.6
	16	190	104	1.7
	32	191	104	3.1
	64	196	107	0.29
Human serum individual 2	2	170	93	8.1
	4	178	97	2.2
	8	183	99	3.7
	16	193	105	0.40
	32	193	105	6.0
	64	200	109	4.7

Parallelism

Parallelism tests could not be performed since the endogenous level of human IL-1 β was below the quantification range. It is recommended that end users assess parallelism when suitable samples with significant levels of analyte are identified.

MATERIALS AND METHODS

The assay was developed on a Gyrolab xP system using Gyrolab® Bioaffy™ 4000 CD. The assay was set up using a three-step method with two wash solutions (4000-3W-001-A) and a 5% PMT setting. The assay buffer was Rexpip H. The Minimum Required Dilution (MRD) for serum samples was 1:2. Mouse monoclonal anti-human IL-1 β antibody (clone 2805) from R&D Systems was biotinylated according to the Gyrolab biotinylation protocol (Gyrolab User Guide) and used in a concentration of 100 μ g/mL, diluted with PBS-T.

The detection antibody, labeled with Alexa Fluor® 647 according to the Gyrolab standard protocol (Gyrolab User Guide), was the goat polyclonal anti-human IL-1 β antibody from R&D Systems, diluted to 50 nM in Rexpip F. The assay standard used was recombinant human IL-1 β , from R&D Systems (catalogue no. 201-LB-005). The standard curve was prepared in Rexpip H.

Summary table

Capture	Mouse monoclonal anti-human IL-1 β antibody (clone 2805, R&D Systems, MAB601-100), biotinylated and diluted to 100 μ g/mL in PBS-T
Detection	Goat polyclonal anti-human IL-1 β antibody (R&D Systems, AF-201-NA) labeled with Alexa Fluor® 647, 50 nM in Rexpip® F
Analyte	Recombinant human IL-1 β (R&D Systems, 201-LB-005) in Rexpip® H
CD-type	Gyrolab® Bioaffy™ 4000
Method	4000-3W-001-A
Wash buffer for needles	Wash buffer 1: PBS-T Wash buffer 2: Gyrolab Wash Buffer pH 11
PMT-setting	5%
Expected dynamic range	Approximately 1 pg/mL to 1 000 pg/mL (2 pg/mL to 2 000 pg/mL in neat human serum, dilution 1:2)

Recommendations

When developing this assay it is important to screen matrices and assess backgrounds, in particular for the specific disease matrices. Parameters, such as LLOQ, should be validated in-house. Data given in this document should only be considered as guidance.

For additional support contact your local Field Application Support